

CROSS-POLARIZATION OPTICAL COHERENCE TOMOGRAPHY PROBES FOR INTRAOPERATIVE APPLICATION IN NEUROSURGERY

K.S. Yashin¹, P.A. Shilyagin^{2*}, E.B. Kiseleva^{2,3}, G.G. Gelikonov², V.N. Romashov², A.A. Moiseev², I.A. Medyanik¹, S.Y. Ksenofontov², K.A. Achkasova³, L.Y. Kravets¹, N.D. Gladkova³

¹ Privolzhsky Research Medical University, University Clinic, 18/1 Verchnevolzhskaya nab., Nizhny Novgorod, 603950, Russia;

² Institute of Applied Physics, Russian Academy of Sciences, 46 Ulyanova St., Nizhny Novgorod, 603950, Russia;

³ Privolzhsky Research Medical University, Institute of Experimental Oncology and Biomedical Technologies, 3 Meditsinskaya St., Nizhny Novgorod, 603104, Russia.

* Corresponding author: paulo-s@mail.ru

Abstract. Optical coherence tomography (OCT) is one of the most promising, innovative and rapidly emerging intraoperative imaging modalities for neurosurgical guidance by brain tissue imaging, «optical biopsy», brain cerebral vascular detection, nerve fibers and white matter tracts detection. In this article, we provide a short survey of cross-polarization OCT and different types of OCT probes that can be used in routine neurosurgical practice. Through different types of probes there are multiple applications where OCT can play a highly complementary role in offering the real-time microscopic assessment and imaging of normal and pathological brain tissues. The biopsy-needle based probe for CP OCT was shown as an effective instrument for brain tissue mapping and express estimation of tissue status as well as for detecting large blood vessels to prevent causing bleeding during biopsy sampling. The folded CP OCT probe for intraoperative use for brain tissue examination was shown as a potentially efficient sensor head for CP OCT. The probe demonstrated high lateral resolution in diffractive limited probing beam quality. The length of the dismountable probe tip allows using the probe under operating microscope. The designed family of specialized probes allows CP OCT to occupy a niche of devices for express brain tissue examination in situ after finishing of the improvement for clinical use process.

Keywords: cross-polarization optical coherence tomography, cross-scattering, probes, brain tumors, stereotactic biopsy, neurosurgical guidance.

List of Abbreviations

OCT – optical coherence tomography

CP OCT – cross-polarization optical coherence tomography

SD OCT – spectral-domain optical coherence tomography

IAP RAS – Institute of Applied Physics of the Russian Academy of Sciences

Introduction

Optical coherence tomography (OCT) is one of the most promising, innovative and rapidly emerging intraoperative imaging modalities for neurosurgical guidance by brain tissue imaging, «optical biopsy», brain cerebral vascular detection, nerve fibers and white matter tracts detection (Fan *et al.*, 2018). OCT imaging has some advantages in the field of intraoperative technologies in neurosurgery: high-resolution, high-speed, low-cost, label free, non-invasiveness, and convenience performance. Several

studies have shown that OCT can provide differentiation between tumorous and non-tumorous tissues through both qualitative (Böhringer *et al.*, 2009; Yashin *et al.*, 2019a) and quantitative assessment (Kut *et al.*, 2015; Yashin *et al.*, 2019b) of the OCT signal by building color-coded maps. Moreover, OCT seems to be an excellent method of myelin visualization, that can be realized using so-called OCT functional extensions – polarization-sensitive (PS) OCT and also polarization-sensitive optical coherence microscopy (Boas *et al.*, 2017; Wang *et al.*, 2016) and cross-polarization (CP) OCT (Yashin *et al.*, 2019a). These OCT modalities provide contrast imaging of myelinated fibers due to their sensitivity to tissue birefringence. Thus, PS OCT allows visualizing white matter tracts in the brain.

There are several scenarios how OCT can be implemented in neurosurgery: (1) OCT can be used intraoperatively for brain imaging and

provide real-time feedback to the surgeons, e.g. clarifying the boundaries of the infiltrative brain tumors within surrounding tissues; (2) OCT can be used for emergency biopsy by neuropathologist; (3) OCT can aid in stereotactic procedures for verifying target for deep brain stimulation or guiding biopsy overcoming challenges both with requirement of multiple sampling and hemorrhagic complications.

According to this possible implementations following OCT scanner designs have been offered: (1) hand-held imaging probes (Garzon-Muvdi *et al.*, 2017; Yashin *et al.*, 2019a), surgical instrumentation (e.g. biopsy needle) (Liang *et al.*, 2011; Pichette *et al.*, 2015; Ramakonar *et al.*, 2018), microscope-integrated systems (Böhringer *et al.*, 2009; Finke *et al.*, 2012; Lankenau *et al.*, 2007) and nonportable stationary OCT systems (Bizheva *et al.*, 2007; Yashin *et al.*, 2019b). However, considering multifunctionality of OCT in neurosurgery the multipurpose device with particular set of OCT probes can be preferred. Moreover, all of using probes need to be driven for optimal surgical ergonomics and compliance with current neurosurgical protocols and other surgical devices in operating room.

This article is devoted to the description of the features of the use of CP OCT devices developed at the IAP RAS in the period 2009-2020 for intraoperative use in surgery for brain tumor pathologies. The material includes a brief overview of the CP OCT technology and systems used to register the CP OCT signal, as well as a description of the main types of scanning units that perform probing of target tissues and organs.

Cross-polarization OCT is a variant of polarization-sensitive OCT

Intensity-based OCT has demonstrated significant results in detecting pathological changes in tissues with layered structure, such as those in the eye. In case of structureless tissue types (brain, breast) the advanced contrast OCT imaging can be achieved by using PS OCT (Baumann, 2017). This technique can detect a number of characteristics of the matter caused by optical anisotropy of its constituent

elements, that provides the possibility to generate tissue-specific contrast (Baumann, 2017; de Boer *et al.*, 2017) in OCT images. Based on the polarization anisotropy of the tissue structure, PS OCT provides better visualization of elongated structures and therefore offers advanced imaging of myelinated fibers in peripheral nerves and the brain (Wang *et al.*, 2016). CP OCT has been shown as a simplified variant of PS OCT providing not only conventional OCT imaging but also allowing visualization of those locations in object where the initial polarization state of the probing light alters into orthogonal state due to birefringence or/and cross-scattering in biological tissues (Gubarkova *et al.*, 2016). This OCT modality enables recording two co-registered images common scattering (conventional OCT image or so-called image in co-polarization) and anisotropic (image in cross-polarization) that detects tissue backscattering producing polarization state orthogonal to the incident one. The last is obtained through the use of the orthogonally polarized backscattered light, which is mutually coherent with the incident one, what contributes to the cross-polarized OCT image. The origin of such “coherent backscattering” includes random polarization during light propagation in the media, depolarization during the backscattering process, and “regular” polarization changes associated with propagation back and forth in birefringent media (Schmitt & Xiang, 1998).

Cross-polarization OCT devices were used

Since 2002 several generations of CP OCT devices with cross-polarization detection were developed in the Institute of Applied Physics of the Russian Academy of Sciences (Nizhny Novgorod, Russia) and produced for custom use by Biomedtech LLC (Nizhny Novgorod, Russia) (Gelikonov *et al.*, 2009; Moiseev *et al.*, 2013), as listed in Table 1 and shown in Figure 1 a, b.

The early studies were performed with the time-domain (TD) CP OCT device «OCT-1300U» (1310 nm wavelength, 200 A-scans per second line rate). The device belongs to a family of endoscope compatible systems, which

Table 1

Cross-polarization OCT devices

	Time-domain OCT-1300U	Spectral-domain CP OCT system
Technical		
Wavelength	1310 nm	1310 nm
Spectrum width	100 nm	120 nm
Scanning rate	200 A-scans/s	20,000 A-scan/s
Probing beam polarization state	random	circular
Acquisition time	2 sec (2D)	0.05 sec (2D), 26 sec (3D for multi-modal)
Image modalities		
2D	yes	yes
3D	no	yes
OCT angiography	no	yes
OCT elastography	no	yes
OCT image analysis		
qualitative	yes	yes
quantitative	only for co-channel, 1 optical coefficient	for co- and cross- channels, several optical coefficients
Approval for clinical use	since 2005	in progress

was approved for clinical use (product license № FCP 2012/13479 from 30 May 2012). It is characterized by number of features that are sufficient for solving the majority of endoscopic tasks, e.g. express estimation of tissue state in small areas. However, the imaging rate and scanning protocol (only the 2D scanning is rational to be used due to low line rate) are out of modern requirements and cannot accomplish the tasks like angiography, elastography, or tissue structure orientation imaging (Moiseev *et al.*, 2019; Sirotkina *et al.*, 2016). The CP OCT image includes both images: (1) cross-polarization (upper part); (2) co-polarization (lower part), as shown in Figure 1 c6.

The spectral-domain (SD) OCT engine for CP OCT imaging was developed in IAP RAS preserving optical characteristics of probing light (central wavelength 1300 nm, output power 5–15 mW). The probing beam bandwidth is little higher than in previously used TD CP OCT device, which causes the lateral resolution of 15 μm in air. The device was designed to provide 20 000 A-scan/s line rate using linear photodiode array SU-512LDB-1.7T1 (Goodrich), 1200 lpmm diffractive

grating T-1200-1310 (LightSmyth) and double prism corrector made from custom crafted elements (Nanyang Jingliang optical technology corp, China). This allowed to avoiding any polarization anisotropy in the spectrometer. To realize uniform optimal conditions for cross-polarization studies of biological tissue the device was equipped with system of active maintenance of the circular polarization of a probing wave in common path OCT setup (Gelikonov *et al.*, 2018). The resulting CP OCT image also includes both co-and cross-images but in reverse order to the ones in TD OCT: (1) co-polarization (upper part); (2) cross-polarization (lower part), as demonstrated in Figure 1c3. The image acquisition can be performed in contact or contactless mode (probe dependent).

Cross-polarization OCT image analysis

Numbers of studies demonstrate that OCT images assessment can be performed through three main approaches: (1) qualitative (visual); (2) quantitative using optical coefficients calculation and (3) combined based on building color-coded maps.

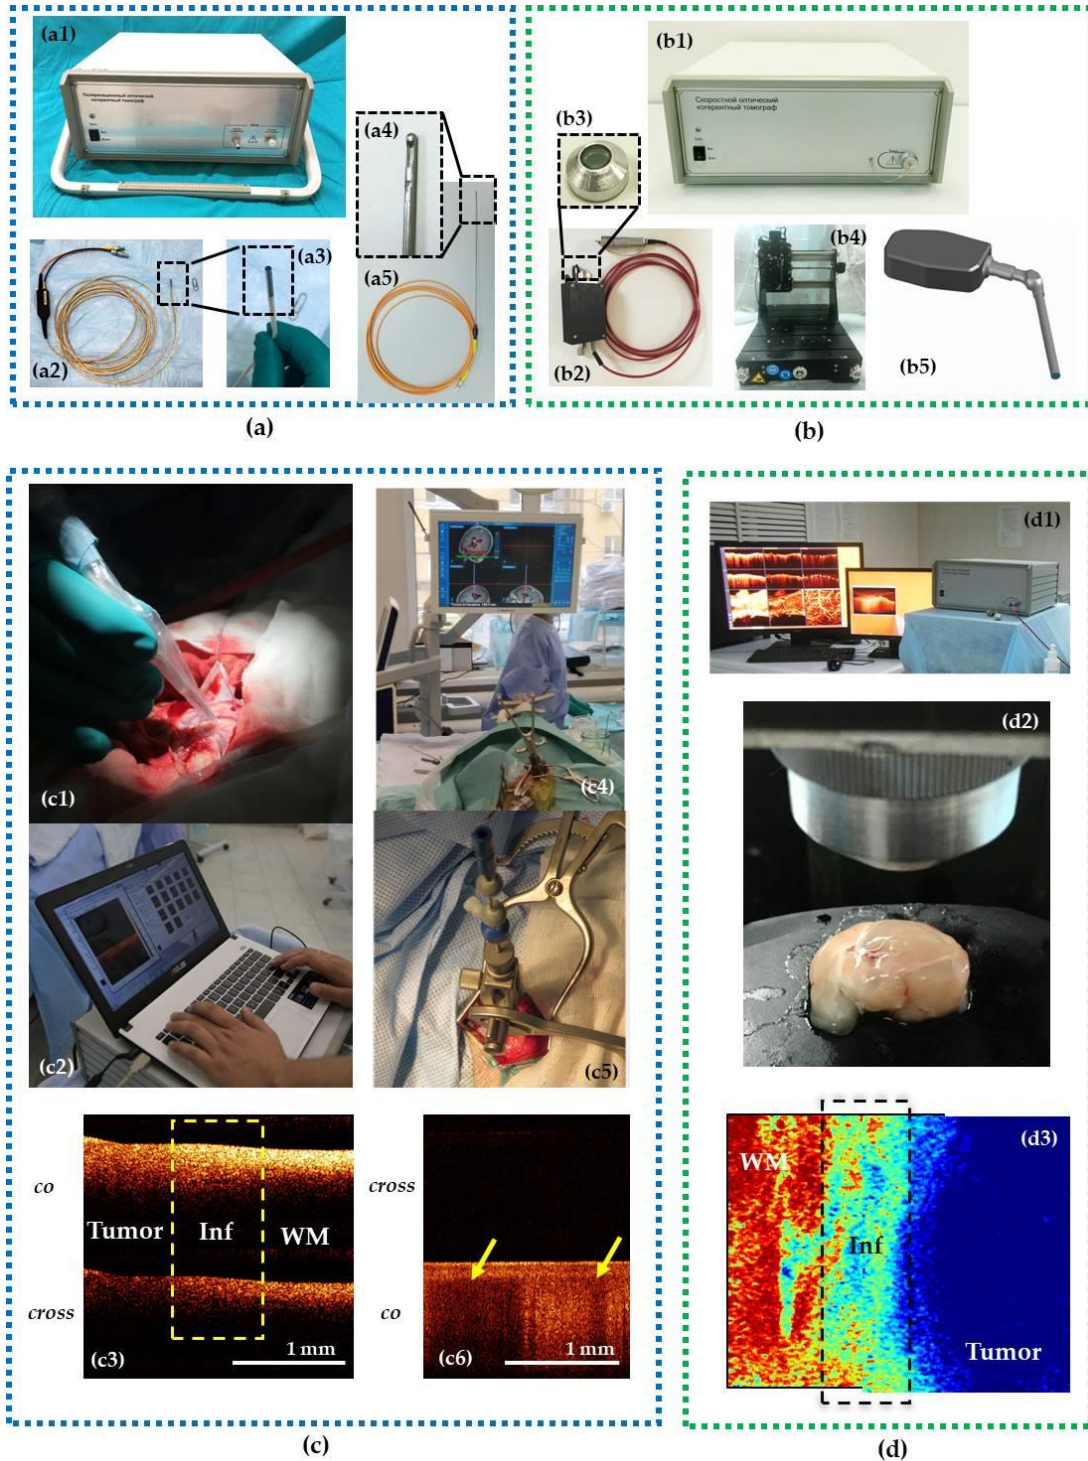


Fig. 1. Different CP OCT devices with compatible probes (a, b) are presented with corresponding types of the CP OCT images in co-polarization and cross-polarization (c3), (c6) and optical coefficient color-coded map (d3). (c3), (d3) CP OCT images demonstrate clear signal differences between tumor and white matter (WM), yellow and black dotted rectangles indicate infiltration zone (Inf) of white matter. (a) Time-domain certified CP OCT device “OCT-1300U” with 2 probes: (a2), (a3) forward- flexible hand-held probe for intraoperative use (c1), (c2) providing 2D images (c3); (a4), (a5) needle-like probe for stereotactic biopsy providing 1D imaging (c6) (yellow arrows are showing the blood vessels) and its possible application during frameless stereotactic biopsy using neuronavigation system (c4), (c5). (b) Spectral-domain OCT device (b1), (d1) with flexible contactless multifunctional CP OCT probes for 3D scanning (b2), (b3), (d2) that can provide user with color-coded maps (d3); (b4) rigid attachment of a probe on a special positioner mount for large area scanning; (b5) the end part of the probe is constructed in curve shape for intraoperative use in the field of an operating microscope

Qualitative assessment is based on visual analysis of light attenuation profile in the tissue in cross-sectional OCT images. This method allows differentiation between tumorous and non-tumorous tissues based on signal intensity parameter as the most powerful criteria (Böhringer *et al.*, 2009; Yashin *et al.*, 2019a). The tumorous tissue is characterized by low signal level and white matter – by high-intensity signal, as shown in Figure 1c3. The key structural element of white matter influencing on features of the received CP OCT signal is the presence of myelin fibers - highly elongated conducting objects. They are responsible for high depolarizing properties demonstrated by white matter in case of fibers chaotic arrangement on the scale of the probing beam while ordered arrangement of myelin fibers causes the origin of linear birefringence and polarizing properties. The qualitative approach provided high sensitivity of (82–85%), specificity (92–94%), and diagnostic accuracy (87–88%) for distinguishing white matter from tumor tissue (Yashin *et al.*, 2019a).

The quantitative approach based on some optical coefficients calculation is seemed to be more objective and accurate method for OCT data analysis. Different strategies for numerical data obtaining were developed, however, it still requires further studies (Kut *et al.*, 2015; Yashin *et al.*, 2019b). The most widespread optical coefficient being used for quantitative processing of OCT signal received from various brain tissues is attenuation coefficient. The sensitivity and specificity of quantitative approach approximate 100% (Kut *et al.*, 2015; Yashin *et al.*, 2019b).

The combined approach includes building of contrast color-coded maps (en-face view on the tissue) representing their values distribution throughout the image (Kut *et al.*, 2015; Yashin *et al.*, 2019b) and in case of gliomas has shown clear differences between tumorous tissue and white matter, as shown in Figure 1d3. This approach looks more promising for clinical use due to combination of quantitative approach accuracy and user-friendliness for evaluation by neurosurgeon.

Cross-polarization OCT probes for neurosurgery

The main part of each sensor device is its distal component, which transfers probing radiation (near IR light in the case of OCT) and receives the signal wave. In OCT this role is played by optical probes, which diversity is very wide. In this paper, we will focus on the description of four different CP OCT probes demonstrated the most valuable clinical applicability. In Table 2 a comparison between these CP OCT probes is presented. The first probe is flexible hand-held CP OCT probe for detecting brain tumor margins, supplied as a standard for TD CP OCT device “OCT-1300U”. The second is side-view modification of the flexible hand-held CP OCT probe, designed for the use in conjunction with stereotactic biopsy needle for “optical biopsy” and detection of blood vessels in the region of interest directly following surgical procedure. The third probe was developed as a part of fast SD OCT system, which can be used for fundamental studies and emergency pathomorphological examinations. It was applied for obtaining a large amount of human post-mortem and animal specimens’ images and was widely used in experimental studies. The last probe design highlighted here is dismountable hand-held curved device intended to be used in operating room equipped with operating microscope.

Flexible hand-held CP OCT probe

The flexible hand-held CP OCT probe (Fig. 1 a2, a3, c1) was constructed at early stages of common-path OCT development. The 5 m-long fiber probe was realized in few modifications with outer diameter of scanning head varying from 1.6 mm to 2.7 mm. The probing beam driving mechanism was described in details in Feldchtein *et al.*, 2002. The probe head design affords its compatibility with the most of commercially available endoscopes, but it also may be used independently.

The small head size makes it possible to use the probe in any environment and previously studies have demonstrated its applicability for tumorous tissue detection during brain cancer resection using described qualitative (visual)

Table 2

The performance comparison of CP OCT probes

Characteristics	Standard CP OCT probes		Specialized CP OCT probes	
	Flexible hand-held probe	Contactless multi-functional CP OCT probe	Stereotactic needle-type probe	Dismountable curved hand-held probe
CP OCT device	Time-domain OCT-1300U	Spectral-domain OCT system	Time-domain OCT-1300U	Spectral-domain OCT system
Probe type	forward-looking	forward-looking	side-looking	forward-looking
Contact/Contactless	Contact	Contactless with contact option	Contact	Contact
Outer diameter of the probe	2.7 mm	8 mm	1.65 mm	8 mm
Axial resolution	15 μ m	10 μ m	15 μ m	10 μ m
Lateral resolution	25 μ m	15 μ m	25 μ m	15 μ m
Lateral image size	2D: 1.3x1.4 mm or 200x256 pixels (width x height)	3D: 2.4x2.4x1.35 mm or 512x512x256 pixels (width x length x height)	2D: from 2 to 200 mm length of the single scan	3D: 2.4x2.4x1.35 mm or 512x512x256 pixels (width x length x height)
Portability	yes	no	yes	yes
Intraoperative use	yes	no	yes	yes
Application	«optical biopsy» – differentiation between tumorous and non-tumorous tissues	Fundamental studies and emergency pathomorphological examination	«optical biopsy» blood vessels and tissue type detection	«optical biopsy» – differentiation between tumorous and non-tumorous tissues

CP OCT criteria (Yashin *et al.*, 2019a). However, the positioning of the probe can face several problems due to its flexibility. Moreover, if one needs the scanning pattern stability enough for realization of color-coded maps, OCT angiography or elastography modalities that look promising for application during neurosurgical procedures, it is impossible to use this probe due to inability of 3D scanning mode. The possible solution of this problem is the development of dismountable curved hand-held probe that will be described below.

Stereotactic needle-type probe

Intensity-based OCT has demonstrated significant results in detecting pathological

changes in tissues with layered structure The probe was designed for the use in conjunction with TD CP OCT device «OCT-1300U» to provide the navigation guidance during taking a biopsy. The probe head was created in a side-view mode using previously described ideas (Liang *et al.*, 2011; Lorensen *et al.*, 2015; Pichette *et al.*, 2015; Ramakonar *et al.*, 2018).

One of the first ideas of brain imaging through the needle-type OCT probe was published in 2011 and the forward-looking imaging needle implementation to brain imaging was described (Liang *et al.*, 2011). The approach demonstrates high usability but is not applicable for biopsy guidance.

Pichette J et al. reported about the biopsy-needle based design of OCT probe in 2015 (Pichette *et al.*, 2015). They set multiple OCT channels on the outer surface of the needle, making it possible to perform OCT visualization directly during the biopsy sampling. The disadvantage of the method lies in its merit – the sampling stylet window is located in a blind zone of the probe (which may be overcome by the main needle rotation) and the outer part becomes very complex in production.

The most valuable design of the biopsy needle compatible probe was provided by David D. Sampson's group (Ramakonar *et al.*, 2018; Scolaro *et al.*, 2012). The biopsy sampling protocol includes the use of standard biopsy needle cover and two inner items consequently induced into its hole: OCT probe to detect safety-sampling area and standard inner stylet to extract the sample.

We constructed principally the same device: the standard biopsy needle tube was used as a probe head body and a system of GRIN lens, spacer and beam reflecting prism was used to project the fiber tip into the tissue under investigation (Fig. 2). The main differences in our design are the use of the actual inner stylet as a body of the OCT probe, which exit window is filled with optically transparent glue, and abandoning mechanized scanning during the examination. In addition, to redirect radiation towards the exit window, a microprism (item 66-767 from Edmund Optics) was glued to the exit end of the spacer instead of an angled polishing of the spacer fiber. Moreover, since the OCT engine is used with the probe was made as common-path OCT with long length of Fizeau interferometer (distance between the fiber tip and outer lens surface of Flexible hand-held CP OCT probe is 10 mm in air), the same distance was preserved between the fiber tip and outer needle tube surface in a needle-type OCT probe. The last produces several difficulties in probe constructing, but it afforded the probe interchangeability with the flexible hand-held CP OCT probe.

The lateral scanning ability was rejected for this probe. The scanning procedure is performed through manual driving of the scanner

along the needle axis and allows recording almost infinite length of the scan. The last gives the opportunity to map the brain from its surface to the target area and be sure that biopsy window is located exactly in tumor area. At this stage of investigations, we believe that preservation of manual driving of the probe is the most appropriate option due to the possibility of varying the velocity of the probe movement (and lateral direction scale on the OCT image) in a wide range based on operator's experience. The image shadow analysis also provides the possibility of detection of large vessels, which should be not a subject of damage during biopsy taking.

Although several scientific groups have already presented stereotactic biopsy needles (Liang *et al.*, 2011; Pichette *et al.*, 2015; Ramakonar *et al.*, 2018), there is no common lens concerning point of its application – vessel detection and preventing hemorrhage or «optical biopsy» of studied tissue. In our opinion, OCT is excellent technology for both tasks and can improve the results of stereotactic biopsy. The «optical biopsy» performed immediately during the procedure can dramatically decrease the risk of the acquisition of non-informative diagnostic samples outside from the viable tumor volume (such as necrotic/gliosis or normal white matter), which has been reported in up to 24% of stereotactic biopsy series (Dammers *et al.*, 2008; Dammers *et al.*, 2010; Zoeller *et al.*, 2009). Currently, neurosurgeon needs to perform intratumoral serial biopsies followed by intraoperative neuropathological assessment (Dammers *et al.*, 2010; Tilgner *et al.*, 2005). It can improve the diagnostic value and accuracy but is associated with an increased risk of intracranial hemorrhages, which have been reported in 0.3–59.8% of cases (Dammers *et al.*, 2008; Field *et al.*, 2001; Grossman *et al.*, 2005) and considerably contribute to the reported mortality of 3,9% (Dammers *et al.*, 2008; Dammers *et al.*, 2010; Field *et al.*, 2001). Stereotactic OCT probe provides the information of blood vessel presence in biopsy point; thereby, surgeon can change the needle position to avoid vessel damage.

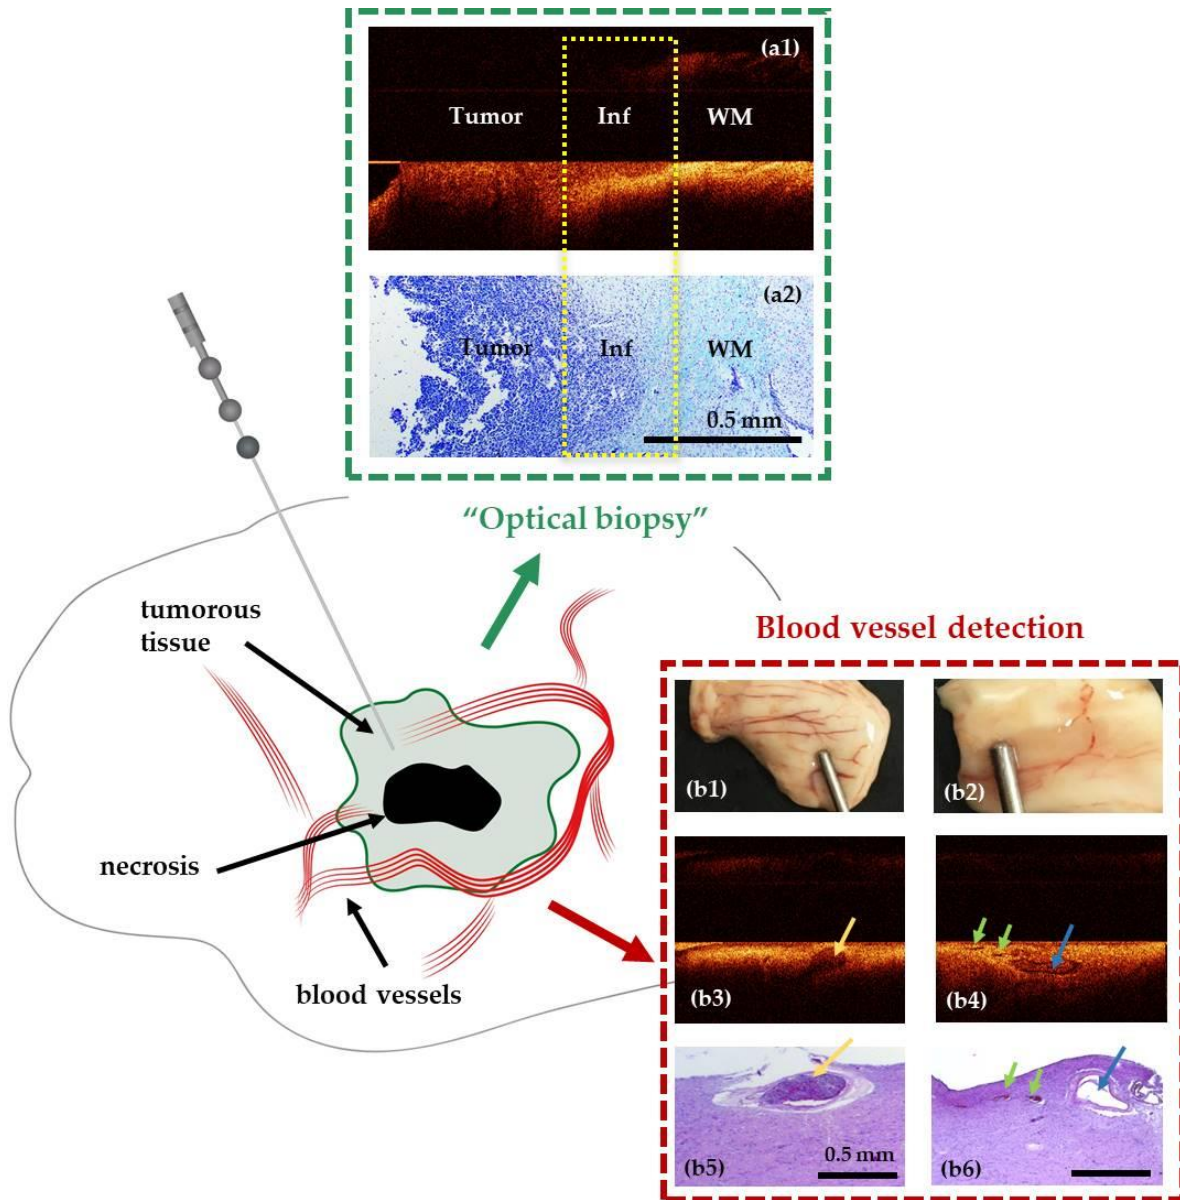


Fig. 2. Stereotactic needle-type OCT probe for vessel detection (b3), (b4) and preventing hemorrhage and “optical biopsy” of studied tissue (a1). The CP OCT images were obtained from rats with astrocytoma 101.8. (a1) Structural CP OCT image demonstrates clear signal differences between tumor and white matter (WM), yellow dotted rectangle indicates infiltration zone (Inf) of white matter. The arrows on CP OCT images and corresponding histological slices show typical CP OCT signs of vessels

Contactless multifunctional CP OCT probe

This probe design does not have any principal differences in comparison with the most of modern 3D MEMS-based OCT probes: it consists of two-axis fast scanning (resonant frequency 340 Hz) MEMS mirror (A8L18.3-4200AU-TINY48.4-B/TP by Mirrorcle Technologies, Inc.) and a simple telecentric scan-

ning lens. The lens is characterized by a relatively short working distance, which allows using the probe in both contact and contactless regimes. The probe body was made to provide compatibility with motorized stage for large area imaging during experiments on animal models or post-mortem samples. The probe demonstrated high potential of 3D CP OCT im-

aging in brain-targeted applications, but its design does not allow using the probe in operating room due to two main factors. Firstly, it is characterized by small length of potentially interchangeable and serializable distal head, which prohibit the use of sterile covers. Secondly, housing profile of the probe is too big for avoiding the overlap of the field of view of operating microscope. While the first problem may be solved by the use of elongated probe head, the second one requires the development of other approaches in constructing of the probe.

This type of probes are widely used in many experimental studies in the field of neurooncology, performed both in vivo and ex vivo on animals and on patients' samples (Assayag *et al.*, 2013; Bizheva *et al.*, 2007; Yashin *et al.*, 2016; Yashin *et al.*, 2019b; You *et al.*, 2020). This type of probe has potential to be a part of optical digital pathomorphological systems with advanced label-based and label-free photonic technologies together along with advances in artificial intelligence, machine learning and computer-aided diagnosis algorithm (Krafft *et al.*, 2018). In particular for neuropathologist OCT can have a powerful impact in the following clinical situations: (1) when excisional biopsy is hazardous and fast real-time feedback for neurosurgeon is required such as following stereotactic biopsy; (2) when pathologists need guidance to select areas of tumor mass in large tissue specimens for histological evaluation such as following temporal lobectomy for diffuse astrocytoma.

Hand-held curved CP OCT probe

Currently two main competitive concepts of using OCT during open neurosurgical procedures have been suggested. On the other hand, the OCT integration into surgical microscope looks the most obviously and comfortable option for surgeon providing wide-OCT imaging directly in oculars (Böhringer *et al.*, 2009; Finke *et al.*, 2012; Lankenau *et al.*, 2007). However, realization of this idea requires the reconstruction of production-release design and building of so-called «OCT-ready» surgical microscope by the developer company. The hand-held imaging probes (Dammers *et al.*, 2010;

Garzon-Muvdi *et al.*, 2017; Yashin *et al.*, 2019a) do not need such technical advances and can be used jointly with microscope for intraoperative assessment of tissues. In brain tumor surgery OCT can be used for in situ detection of cancer tissue via «optical biopsy». However, most of suggested systems are not comfortable in clinical use due to their size, shape, flexibility etc.

The bayonet-shaped CP OCT probe presented in this paper seems to be most favorable option since this construction is familiar for surgeon and preserves field of view, as shown in Figure 3a. The probe consists of two detachable parts – the scanning head with long flexible cable and a group of focusing optics with folded axis contained in a stainless steel tube of complex shape. The focusing optics group is designed from telecentric scanning group (1) and 1:1 translator (3) (Fig. 3b) combined with equilateral prism, which entrance and exit sides are orthogonal to the chief ray of probing beam. The prism glass (BK7) refractive index and the angle of incidence to the reflecting side (60 degrees) cause total internal reflection from this face, therefore, this element does not induce optical losses into the optical path of the device. To minimize flare-blinding effects the exit window of the probe is made of curved inner shape, the outer surface has small tilt (2 degrees) to the optical axis of the probe. In addition to flare repression, the tilted outer surface helps to prevent the appearance of air bubbles when touching an uneven elastic surface by squeezing the latter over the edge of the window.

Long focal lens using in the optical setup provides paraxial beam propagation and causes diffraction limited quality of the beam in its focal plane. The optical setup provides 15 μm axial resolution while the Rayleigh length is about 0.5 mm. The system is achromatized for 1250-1350 nm optical range, the image distortion not exceed 0.5% value.

The optic group connection is made based on of LEMO's® Push-Pull Self-Latching Connection System (not shown in detail of Fig. 3), well known by the most of clinicians. The length of dismountable probe tip is 150 mm that is

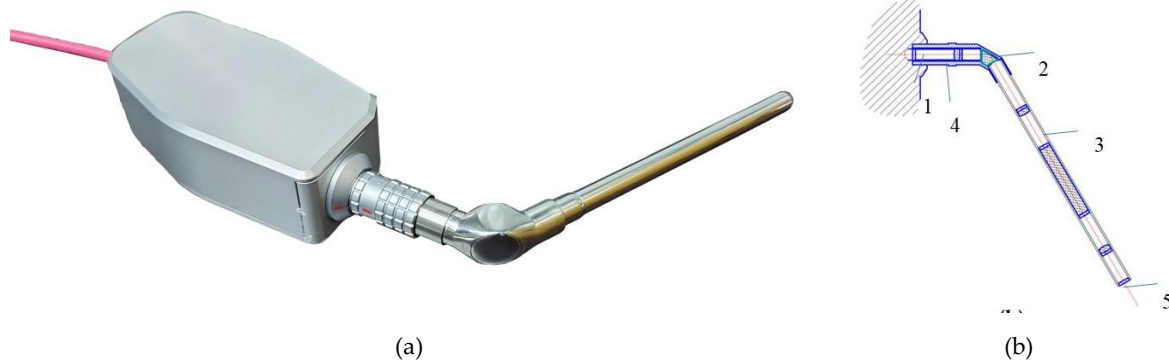


Fig. 3. Optical setup of bayonet-shaped probe for CP OCT: (a) external view; (b) schematic and. 1 – telecentric scanning lens group, 2 – probe folding, 3 – replaceable sterilizable optical beam translator, 4 – standard LEMO's® coupling, 5 – main optical axis

enough to provide the possibility to use it conjunctly with operating microscope.

Due to the use of LEMO's® connection the distal part of the probe may be easily dismounted and then sterilized using one of standard protocols based on chemical solutions or gas methods applicable for endoscope systems including STERRAD. The prohibited sterilizing methods include usage of solutions containing hydrogen peroxide (concentration 6% or more), formic acid and other strong oxidants, incl. ozone. With all methods of disinfection and sterilization, the temperature should not exceed 100 degrees Celsius, sudden changes in temperature are also not allowed. The probe scanning head with its flexible connection cable may be treated with disinfectant solutions but it should be enclosed in sterile cover while in the operating room.

Conclusions

Recently studies have been shown that OCT has a great potential in neurosurgery the best known in brain tumor surgery. As described here through different types of probes there are multiple applications where OCT can play a highly complementary role in offering the real-time microscopic assessment and imaging of tissues during brain tumor surgery, stereotactic biopsy and in the pathology laboratory. The biopsy-needle based probe for CP OCT was

shown as an effective instrument for brain tissue mapping and express estimation of tissue status as well as for detecting large blood vessels to prevent causing bleeding during biopsy sampling. The folded CP OCT probe for intraoperative use for brain tissue examination was shown as a potentially efficient sensor head for CP OCT. The probe demonstrated high lateral resolution in diffractive limited probing beam quality. The length of dismountable probe tip allows using the probe under operating microscope. The designed family of specialized probes allows CP OCT to occupy a niche of devices for express brain tissue examination in situ after finishing of the approval for clinical use process.

Conflicts of interest: the authors declare no conflict of interest.

Funding: this research was funded by the State Task of IAP RAS (Project No. 0030-2021-0013).

Acknowledgements

The authors express their deep gratitude to Dr. Nikolay N. Karyakin (rector of PRMU, Nizhny Novgorod, Russia) for active supporting translation of CP OCT into clinical usage. We also thank the Maria Chugrina for her help with the design of figures.

References

- ASSAYAG O., GRIEVE K., DEVAUX B., HARMS F., PALLUD J., CHRETIEN F., BOCCARA C. & VARLET P. (2013): Imaging of non-tumorous and tumorous human brain tissues with full-field optical coherence tomography. *NeuroImage. Clinical* **2**, 549-557.
- BAUMANN B. (2017): Polarization Sensitive Optical Coherence Tomography: A Review of Technology and Applications. *Applied Sciences* **7**(5), 474.
- BIZHEVA K., UNTERHUBER A., HERMANN B., POVAZAY B., SATTMANN H., FERCHER A., DREXLER W., PREUSSER M., BUDKA H., STINGL A. & LE T. (2007): Imaging ex vivo healthy and pathological human brain tissue with ultra-high-resolution optical coherence tomography. *Journal of Biomedical Optics* **10**(1), 011006.
- BOAS D.A., WANG H., MAGNAIN C. & FISCHL B. (2017): Polarization-sensitive optical coherence tomography of the human brain connectome. *SPIE Newsroom* (27 January 2017).
- BÖHRINGER H.J., LANKENAU E., STELLMACHER F., REUSCHE E., HÜTTMANN G. & GIESE A. (2009): Imaging of human brain tumor tissue by near-infrared laser coherence tomography. *Acta Neurochirurgica* **151**(5), 507-517.
- DAMMERS R., HAITSMAN I.K., SCHOUTEN J.W., KROS J.M., AVEZAAT C.J.J. & VINCENT A.J.P.E. (2008): Safety and efficacy of frameless and frame-based intracranial biopsy techniques. *Acta Neurochirurgica* **150**(1), 23-29.
- DAMMERS R., SCHOUTEN J.W., HAITSMAN I.K., VINCENT A.J.P.E., KROS J.M. & DIRVEN C.M.F. (2010): Towards improving the safety and diagnostic yield of stereotactic biopsy in a single centre. *Acta Neurochirurgica* **152**(11), 1915-1921.
- DE BOER J.F., HITZENBERGER C.K. & YASUNO Y. (2017): Polarization sensitive optical coherence tomography - a review [Invited]. *Biomedical optics express* **8**(3), 1838-1873.
- FAN Y., XIA Y., ZHANG X., SUN Y., TANG J., ZHANG L. & LIAO H. (2018): Optical coherence tomography for precision brain imaging, neurosurgical guidance and minimally invasive theranostics. *BioScience Trends* **12**(1), 12-23.
- FELDCHEIN F.I., GELIKONOV V.M. & GELIKONOV V.M. (2002): Design of OCT Scanners. In: *Handbook of Optical Coherence Tomography* (Eds Bouma B.E. & Tearney G.J.), pp. 125-142. New York, Basel: Marcel Dekker, Inc.
- FIELD M., WITHAM T.F., FLICKINGER J.C., KONDZIOLKA D. & LUNSFORD L.D. (2001): Comprehensive assessment of hemorrhage risks and outcomes after stereotactic brain biopsy. *Journal of Neurosurgery* **94**(4), 545-551.
- FINKE M., KANTELHARDT S., SCHLAEFER A., BRUDER R., LANKENAU E., GIESE A. & SCHWEIKARD A. (2012): Automatic scanning of large tissue areas in neurosurgery using optical coherence tomography. *The International Journal of Medical Robotics and Computer Assisted Surgery* **8**(3), 327-336.
- GARZON-MUVDI T., KUT C., LI X. & CHAICHANA K.L. (2017): Intraoperative imaging techniques for glioma surgery. *Future Oncology* **13**(19), 1731-1745.
- GELIKONOV V.M., GELIKONOV G.V. & SHILYAGIN P.A. (2009): Linear-wavenumber spectrometer for high-speed spectral-domain optical coherence tomography. *Optics and Spectroscopy* **106**(3), 459-465.
- GELIKONOV V.M., ROMASHOV V.N., SHABANOV D.V., KSENOFONTOV S.Y., TERPELOV D.A., SHILYAGIN P.A., GELIKONOV G.V. & VITKIN I.A. (2018): Cross-Polarization Optical Coherence Tomography with Active Maintenance of the Circular Polarization of a Sounding Wave in a Common Path System. *Radiophysics and Quantum Electronics* **60**(11), 897-911.
- GROSSMAN R., SADETZKI S., SPIEGELMANN R. & RAM Z. (2005): Haemorrhagic complications and the incidence of asymptomatic bleeding associated with stereotactic brain biopsies. *Acta Neurochirurgica* **147**(6), 627-631.
- GUBARKOVA E.V., DUDENKOVA V.V., FELDCHEIN F.I., TIMOFEEVA L.B., KISELEVA E.B., KUZNETSOV S.S., SHAKHOV B.E., MOISEEV A.A., GELIKONOV V.M., GELIKONOV G.V., VITKIN A. & GLADKOVA N.D. (2016): Multi-modal optical imaging characterization of atherosclerotic plaques. *Journal of Biophotonics* **9**(10), 1009-1020.
- KRAFFT C., VON EGGELING F., GUNTINAS-LICHIUS O., HARTMANN A., WALDNER M.J., NEURATH M.F. & POPP J. (2018): Perspectives, potentials and trends of ex vivo and in vivo optical molecular pathology. *Journal of Biophotonics* **11**(1), e201700236.

- KUT C., CHAICHANA K.L., XI J., RAZA S. M., YE X., MCVEIGH E.R., RODRIGUEZ F.J., QUIÑONES-HINOJOSA A. & LI X. (2015): Detection of human brain cancer infiltration ex vivo and in vivo using quantitative optical coherence tomography. *Science translational medicine* **7**(292), 292ra100-292ra100.
- LANKENAU E., KLINGER D., WINTER C., MALIK A., MÜLLER H.H., OELCKERS S., PAU H.-W., JUST T. & HÜTTMANN G. (2007): Combining Optical Coherence Tomography (OCT) with an Operating Microscope. In: *Advances in Medical Engineering* (Eds Buzug T.M., Holz D., Bongartz J., Kohl-Bareis M., Hartmann U. & Weber S.), pp. 343-348. Berlin, Heidelberg: Springer Berlin Heidelberg.
- LIANG C.-P., WIERWILLE J., MOREIRA T., SCHWARTZBAUER G., JAFRI M.S., TANG C.-M. & CHEN Y. (2011): A forward-imaging needle-type OCT probe for image guided stereotactic procedures. *Optics express* **19**(27), 26283-26294.
- LORENSER D., MCLAUGHLIN R.A. & SAMPSON D.D. (2015): Optical Coherence Tomography in a Needle Format. In: *Optical Coherence Tomography: Technology and Applications* (Eds Drexler W. & Fujimoto J.G.), pp. 2413-2472. Cham: Springer International Publishing.
- MOISEEV A.A., GELIKONOV G.V., TERPELOV D.A., SHILYAGIN P.A. & GELIKONOV V.M. (2013): Noniterative method of reconstruction optical coherence tomography images with improved lateral resolution in semitransparent media. *Laser Physics Letters* **10**(12), 125601.
- MOISEEV A.A., KSENOFONTOV S.Y., TERPELOV D.A., KISELEVA E.B., YASHIN K.S., SIROTKINA M.A., GLADKOVA N.D. & GELIKONOV G.V. (2019): Optical coherence angiography without motion correction preprocessing. *Laser Physics Letters* **16**(4), 045601.
- PICHETTE J., GOYETTE A., PICOT F., TREMBLAY M.-A., SOULEZ G., WILSON B. C. & LEBLOND F. (2015): Sensitivity analysis aimed at blood vessels detection using interstitial optical tomography during brain needle biopsy procedures. *Biomedical optics express* **6**(11), 4238-4254.
- RAMAKONAR H., QUIRK B.C., KIRK R.W., LI J., JACQUES A., LIND C.R.P. & MCLAUGHLIN R.A. (2018): Intraoperative detection of blood vessels with an imaging needle during neurosurgery in humans. *Science advances* **4**(12), eaav4992-eaav4992.
- SCHMITT J.M. & XIANG S.H. (1998): Cross-polarized backscatter in optical coherence tomography of biological tissue. *Optics Letters* **23**(13), 1060-1062.
- SCOLARO L., LORENSER D., MCLAUGHLIN R.A., QUIRK B.C., KIRK R.W. & SAMPSON D.D. (2012): High-sensitivity anastigmatic imaging needle for optical coherence tomography. *Optics Letters* **37**(24), 5247-5249.
- SIROTKINA M.A., KISELEVA E.B., GUBARKOVA E.V., BUYANOVA N.L., ELAGIN V.V., ZAITSEV V.Y., MATVEEV L.A., MATVEEV A.L., KIRILLIN M.Y., GELIKONOV G.V., GELIKONOV V.M., KUZNETSOV S.S., ZAGAYNOVA E.V. & GLADKOVA N.D. (2016): Multimodal optical coherence tomography in the assessment of cancer treatment efficacy. *Bulletin of RSMU* **4**, 19-26.
- TILGNER J., HERR M., OSTERTAG C. & VOLK B. (2005): Validation of Intraoperative Diagnoses Using Smear Preparations from Stereotactic Brain Biopsies: Intraoperative versus Final Diagnosis—Influence of Clinical Factors. *Neurosurgery* **56**(2), 257-265.
- WANG H., AKKIN T., MAGNAIN C., WANG R., DUBB J., KOSTIS W.J., YASEEN M.A., CRAMER A., SAKADŽIĆ S. & BOAS D. (2016): Polarization sensitive optical coherence microscopy for brain imaging. *Optics Letters* **41**(10), 2213-2216.
- YASHIN K., GUBARKOVA E.V., KISELEVA E.B., KUZNETSOV S.S., KARABUT M.M., TIMOFEEVA L.B., GLADKOVA N.D., SNOPOVA L.B., MOISEEV A.A., MEDYANIK I.A. & KRAVETS L.Y. (2016): Ex vivo Visualization of Human Gliomas with Cross-Polarization Optical Coherence Tomography: Pilot Study. *Sovremennye tehnologii v medicine* **4**, 14-21.
- YASHIN K. S., KISELEVA E.B., GUBARKOVA E.V., MOISEEV A.A., KUZNETSOV S.S., SHILYAGIN P.A., GELIKONOV G.V., MEDYANIK I.A., KRAVETS L.Y., POTAPOV A.A., ZAGAYNOVA E.V. & GLADKOVA N.D. (2019a): Cross-Polarization Optical Coherence Tomography for Brain Tumor Imaging. *Frontiers in oncology* **9**, 201-201.
- YASHIN K.S., KISELEVA E.B., MOISEEV A.A., KUZNETSOV S.S., TIMOFEEVA L.B., PAVLOVA N.P., GELIKONOV G.V., MEDYANIK I.A., KRAVETS L.Y., ZAGAYNOVA E.V. & GLADKOVA N.D. (2019b): Quantitative nontumorous and tumorous human brain tissue assessment using microstructural co- and cross-polarized optical coherence tomography. *Scientific Reports* **9**(1), 2024.

- YOU J., PAN C., PARK K., LI A. & DU C. (2020): In vivo detection of tumor boundary using ultrahigh-resolution optical coherence angiography and fluorescence imaging. *Journal of Biophotonics* **13**(3), e201960091-e201960091.
- ZOELLER G.K., BENVENISTE R.J., LANDY H., MORCOS J.J. & JAGID J. (2009): Outcomes and management strategies after nondiagnostic stereotactic biopsies of brain lesions. *Stereotact Funct Neurosurg* **87**, 174–181.